
ORTHOPUS SUPPORTER

QUICKCHART



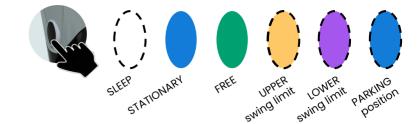

STATIONARY MODE = BLUE

Locks in the height chosen

down



SLEEP MODE

= BLINKING WHITE

2 SHORT CLICKS on the rear button to

go back in SLEEP mode



CHANGE THE MODE

1 LONG CLICK on both buttons of the control pad

OR



1 SHORT CLIC on the rear button

Short vibration = **OK**

SETTING SWING LIMITS










REAR BUTTON' COLORS







1LONG CLICK

Set the **upper** swing limit

Set the lower swing limit

Back in **STATIONARY** mode



Position the device where you would like to set the limit with the control pad



To **SET, I LONG CLICK** Long vibration = **OK**

To skip WITHOUT setting, 1 SHORT CLICK

FREE MODE = GREEN

Accompanies the movements





+100g /clic

SETTING AN IDEAL COMPENSATION FORCE



1 LONG CLICK on the rear button Short vibration = **OK**

PARKING POSITION ON WHEELCHAIR

In **STATIONARY** mode, pull down the ORTHOPUS Supporter on the armrest: the device stays blocked in place.



Rear button **blinking blue**

Parking position activated = **OK**

To go out of the Parking position, click on the + button of the control pad.

WAITING FREE MODE



Rear button **blinking green**

If the device is switched in FREE mode without arm in the arm brace, the ORTHOPUS Supporter puts itself in safety.

ERROR MODE



Unplug the device and wait a few minutes before using it again. If the Rear button stays red, please contact your ORTHOPUS Supporter Country Representative.

RECOMMENDATIONS

- While starting the ORTHOPUS
 Supporter, don't touch the control pad
 and don't install an arm in the arm brace.
- Prior to removing the user's arm from the support, please **always ensure** that the ORTHOPUS Supporter is in STATIONARY or SLEEP mode.
- It is recommended that users **become** acclimated to the device gradually and be monitored by a qualified healthcare professional.
- Only an **individual trained specifically** is authorized to install the ORTHOPUS Supporter.

To take full advantage of all that the ORTHOPUS Supporter has to offer, **please** make sure:

- In horizontal position, the arm isn't leaning forwards or backwards.
- The arm is always in contact with the elbow support. If necessary, set an upper swing limit.
- On the wheelchair, cables and box interface are protected for the rain.

IMPORTANT INFORMATIONS

- 1 You must read the full user manual for the device **orthopus.com/documentation**
- Do not apply excessive force to the device. For example, do not lean on it. **The ORTHOPUS Supporter is designed** solely to support the arm.
- lf there are any defects or damage to the electronic components, do not use the device. Contact your medical equipment provider for any maintenance issues.
- Do not modify any part of this equipment, as this may result in the loss of the warranty.
- The device is resistant to water splashes but is **not waterproof.** Do not expose it to heavy rain, high humidity, or snowfall.



If the ORTHOPUS Supporter isn't mounted, it must remain in its packaging and box at all times. The box is to be kept should the device need to be returned.



ORTHOPUS Supporter Quickchart v1.2 - 2025/03/04